



Aerosol Contamination in the Dental Operator During Oral Prophylaxis: An Occupational Hazard

**Dipika Inbasekaran^a, Jaiganesh Ramamurthy^a, A. S. Smiline Girija^b
and Gopal Nambi^{c*}**

^aDepartment of Periodontics, Saveetha Dental College, Saveetha Institute of Medical and Technical Sciences, Saveetha University, Chennai, India.

^bDepartment of Microbiology, Saveetha Dental College, Saveetha Institute of Medical and Technical Sciences, Saveetha University, Chennai, India.

^cDepartment of Health and Rehabilitation Sciences, College of applied medical sciences, Prince Sattam bin Abdulaziz University, Al Kharj, Saudi Arabia.

Authors' contributions

This work was carried out in collaboration among all authors. All authors read and approved the final manuscript.

Article Information

DOI: 10.9734/JPRI/2021/v33i62A35155

Open Peer Review History:

This journal follows the Advanced Open Peer Review policy. Identity of the Reviewers, Editor(s) and additional Reviewers, peer review comments, different versions of the manuscript, comments of the editors, etc are available here: <https://www.sdiarticle5.com/review-history/82205>

Original Research Article

Received 07 October 2021

Accepted 27 December 2021

Published 28 December 2021

ABSTRACT

Aim: To investigate the level of aerosol contamination following oral prophylaxis using ultrasonic scalers at different positions in the dental operator at different time.

Methodology: In a pre-fumigated room of 10m*15m scaling was performed using ultrasonic scalers along with high volume suction while maintaining all aseptic precautions. Blood agar plates were positioned at the level of patient's chest (P1), doctor's chest (P2), assistant's chest (P3), on the floor directly below the patients headrest (P4) and 4 feet away from the dental chair at a height 3 feet above the ground (P5) to assess aerosol contamination occurring during scaling procedure. Similarly, blood agar plates were positioned at P3, P4, P5 for a time interval of 15 minutes after 1 and 3 hours of the procedure respectively to assess the levels of aerosol post procedure.

All the blood agar plates were incubated at 37°C for 24 hours, following which bacterial colony forming unit (CFU) was calculated for each plate and gram staining was performed to identify the organism present.

Results: At the time of procedure the patient was most exposed to the aerosol. At the end of 3 hours the percentage of aerosol reduction was 81 %. Gram staining showed that the streptococci

were predominant organisms with a few short rods as observed on the plates obtained during the procedure, while gram positive bacilli were seen abundantly in samples obtained at the end of 3 hours.

Conclusion: The study examined the spreading characteristics of aerosol during and after scaling procedure. Even after 3 hours of completion of the procedure some amount of aerosol present in the room. Hence, the dentist must ensure proper precautionary measures to prevent air-borne nosocomial infections.

Keywords: Aerosol; contamination; oral prophylaxis.

1. INTRODUCTION

The human mouth is a highly contaminated environment, the dentist and dental hygienist are exposed to a variety of bacteria, viruses, fungi and protozoan. The dental biofilm contains 2×10^8 microorganisms and over 500 different species [1]. High-powered devices such as airtors and ultrasonic scalers need compressed air and water to work effectively. Procedures performed by the dental team using these devices have the potential for creating contaminated aerosols and splatter.

Aerosols are droplets and or tiny particles which remain suspended in air. The size of the particle varies from 0.001 mm to 100 μm or more. The small particle of size ranging from 0.5 μm to 10 μm have the greatest potential to penetrate the respiratory passages and the lungs, hence, they possessing the ability to transmit diseases [2]. These aerosols are a potential source of infection as they are grossly contaminated with microorganisms and blood. Microorganism present in the mouth and upper respiratory tract can be transported in the aerosol produced during dental procedures such as restorations or scaling, leading to infection of the respiratory system, skin infections and other systemic diseases in immuno-compromised patient [3]. There is some evidence for greater prevalence of respiratory diseases and elevated antibody levels to *Legionella pneumophila* in dental workers [4]. The detection of oral bacteria as far as two meters away from the operatory site is indicative of the existence of aerosolized oral bacteria in dental practice [5]. The use of ultrasonic scalers and highspeed hand pieces are responsible for increased aerosol contamination and decreased air quality in the dental office [6]. Scaling with ultrasonic scalers generate aerosols contain millions of bacteria per cubic foot of air, bacteria could be recovered 6 inches from the mouth of patient and the CFUs formed were significantly reduced when aerosol reduction device are used [7].

Past evidence is available for aerosol contamination due to dental procedures. However, this study is novel because it aims to investigate the level of bacterial contamination by aerosol following oral prophylaxis using ultrasonic scalers in three dimensions: namely at different positions in the dental operatory and at different time levels.

2. MATERIAL AND METHODS

This observational study was conducted from December 2019 to February 2020. The patients required for the study were recruited from the out-patient department of Department of Periodontics, Saveetha Dental College and Hospitals.

A single chaired, closed-operatory measuring 10 feet x 15 feet, with the facility to fumigate the room was chosen for all treatment procedures. A single patient was treated in the room on each of the study day. A total of 5 otherwise healthy patients requiring oral prophylaxis and consenting to be a part of the study were included. A written informed was taken from the patients after explaining the study protocol and explaining that participation was voluntary.

The room was fumigated on the day prior to the day the test patients were treated and all surfaces were cleaned with 2% glutaraldehyde solution. Sodium Hypochlorite (0.5%) was flushed through the tubing of dental chair waterline followed by water flushing to remove the unwanted biofilm from the tubing surfaces. Following fumigation the room was kept closed to maintain sterility. The following morning, on the same day of the procedure, a sterile Petri dish containing blood agar is left on the dental chair for 15 minutes and then immediately incubated for 24 hours at 37°C to assess the sterility of the dental operatory prior to the start of any dental procedure.

The operator as well as the assistant wore sterile surgical gloves, face masks, head caps and used protective eye-glasses throughout the procedure, while the patient wore a sterile surgical drape (Fig. 1).

Using a double-sided tape, sterile blood agar petri dishes were taped onto the chest of the dentist (position P1), assistant (position P2) and patient (position P3). Agar Petri dishes were placed at ground level just below the patient's head (position P4) and at a distance of 4 feet from the dental chair at a height 3 feet above the ground (position P5). A through sub gingival scaling was performed with the speed water settings set at moderate levels. A high vacuum suction was used at all times to aspirate water, saliva and debris collected in the mouth during the procedure. After completion of the procedure the agar plates were immediately labelled and incubated for 24 hours at 37°C to assess the

level of contamination at the baseline or time T0.

After 1 hour, sterile agar plates were placed on the head rest of the dental chair, on the floor directly below the head rest (corresponding to position P4) and at a distance of 4 feet away from the dental chair at a height 3 feet above the ground (corresponding to position P5). The plates were left open for 15 minutes after which the petri dishes were labelled and incubated for 24 hours at 37°C to assess the spread of aerosol after 1 hour of procedure of time T1. The same was repeated after 3 hours of the procedure and the time period was called as T2. The room was kept closed at all time.

All agar plates were incubated for 24 hours at 37°C after which each of the agar plate was examined for colony count, colony morphology and Gram staining was performed to identify the bacteria present (Fig. 2).



Fig. 1. Positioning of agar plates

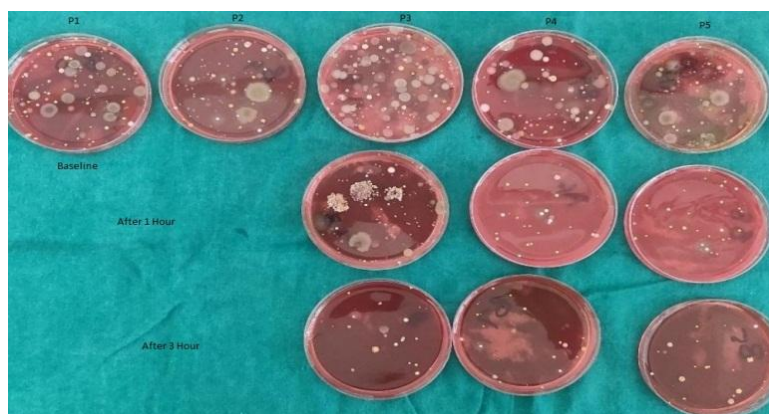


Fig. 2. Agar plates after 24 hours of incubation at 37°C according to position and type

3. RESULTS

The data was collected, tabulated and analyzed. Table 1 depicts mean CFU values for all the patients at different positions at different time intervals. The 5 × 3 (position × time) multivariate analysis shows significant difference in aerosol levels at different positions at different time intervals ($p < 0.001$). At the time of scaling patient (position P3) was most exposed to aerosol, followed by dentist (position P1) and dental assistant (position P2), least amount of aerosol was detected 4 feet away from the dental chair (position P5) (Fig. 3).

Percentage reduction in CFU was calculated at different positions at 1 and 3 hours post scaling. At 1- hour, maximum reduction (67.78%) was seen at the headrest position (position P3) and the percentage reduction from baseline of CFU was 89.07% at position P3 at 3 hours after scaling. Even after 3 hours some amount of aerosol remained suspended in the air (Fig. 4). Gram staining revealed the presence of abundant *streptococci*, *staphylococci*, and few *bacilli* (Fig. 5).

4. DISCUSSION

This study was conducted with the aim to investigate the level of aerosol contamination occurring during scaling procedure in terms of time and distance from the dental chair. Modern dental procedures are associated with aerosol production; in particular, ultrasonic scalers have been reported to generate more aerosols than hand pieces and air-water syringes [8]. Ultrasonic scaling produces a huge volume of aerosol; which apart from air and water, the aerosol contains blood, saliva and microbes

contained in them. These organisms could lead to the occurrence of nosocomial infection in susceptible individuals. With the emergence of newer perio-pathogens, it is very important to treat every patient as a potentially infective patient in our everyday practice.

Patients periodontal status, type of evacuator used and use of preprocedural rinse are some factors which influence aerosol distribution [9]. The use of an ultrasonic scaler is associated with an increase in the prevalence of respiratory disease in dental medical staff [10]. Dentists and dental hygienists who used an ultrasonic scaler for more than 60 min a day showed a higher rate of eye and skin infections [11].

Our study found that the patient followed by the clinician and assistant were in the most contaminated zone, these results were similar too these seen by Veena H R et al who studied aerosol distribution during scaling on a mannequin fitted with phantom jaws on a dental chair [12]. JR Allison et al using fluorescein dyes studied spreading characteristics of aerosol generated by high-speed airturbine, ultrasonic scaler and 3-in-1 spray they concluded that all devices were capable of generating aerosol and that the patient and operator were in the most contaminated zone [13]. Similar to our A. Singh et al in a observed significant increased number of bacterial colonies immediately after scaling with *Streptococci* and *Staphylococci* being the predominant organisms [14]. According to Bennet et al the aerosol remained suspended in the air even after 30 mins, in our study we found that approximately 20% of aerosol still remained suspended in the dental operatory even after 3 hours [15]. Choi et al observed that the use of pre-procedural rinses prior to scaling reduced the aerosol contamination [16].

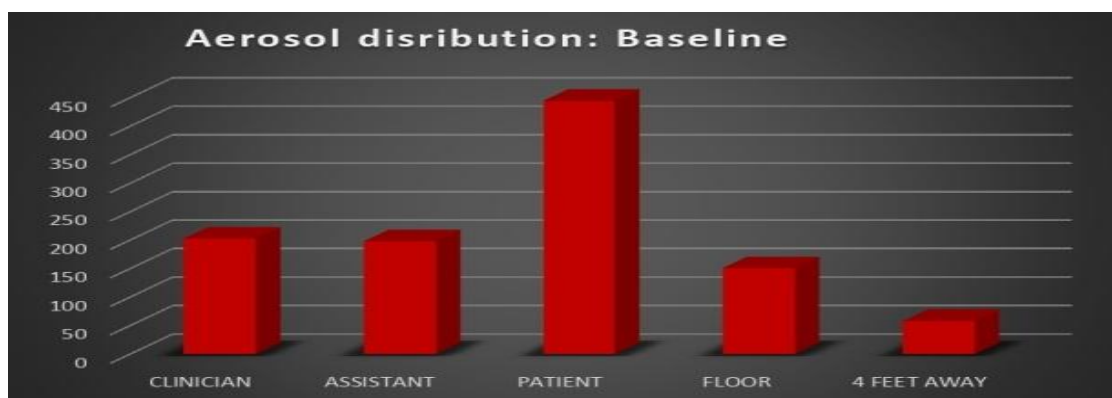


Fig. 3. Baseline distribution of aerosol

Table 1. Distribution of aerosol in different positions at various time intervals

Time	Positions					P value
	P1	P2	P3	P4	P5	
T0:Baseline	203 ± 5.71	181 ± 13.47	469 ± 17.45	141.66 ± 7.03	147 ± 6.16	0.001
T1: After 1 hr	-	-	145.33 ± 7.94	57.33 ± 13.57	60 ± 4.63	
T2: After 3 hr	-	-	53.33 ± 9.84	32.66 ± 8.73	28.33 ± 7.94	

P1 – Dentist, P2 – Assistant, P3 - Patient/ head rest at reclined position, P4 - Floor level below chair head rest at reclined position, P5 - 4 feet away, 3 feet above the ground

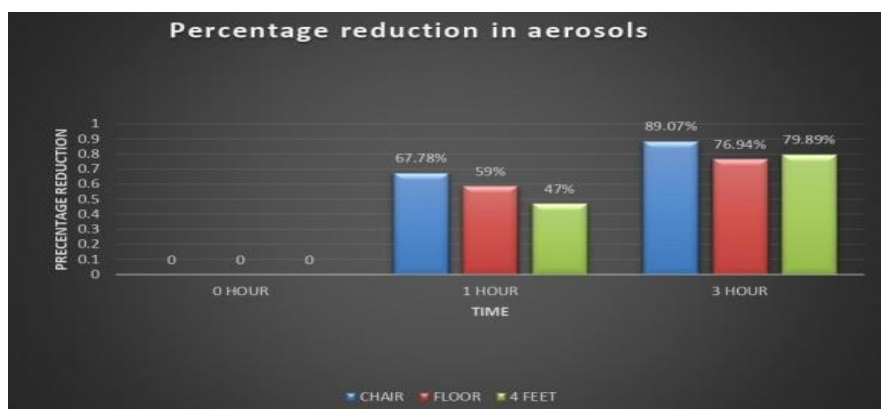


Fig. 4. Percentage reduction from baseline at 1 and 3 hours at different positions

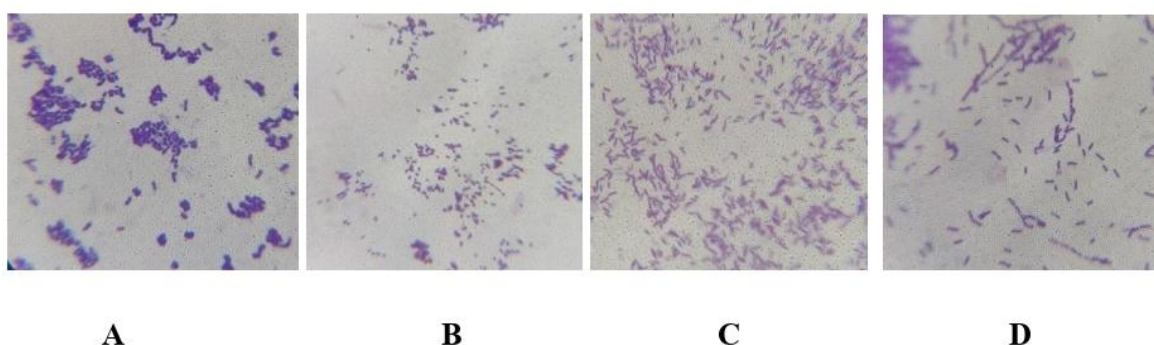


Fig. 5. Gram staining of the organisms cultured. Gram positive cocci in clusters (A), Gram positive cocci in pairs (B), Gram positive bacilli (C) and Gram positive bacilli in chains (D)

The COVID-19 pandemic, where the virus is transmitted through aerosols has shifted the focus on how the dental operator is a highly infectious zone and that measures to prevent infection transmission by aerosols must be implemented as a part of dental practice [17]. In order to protect the dental personnel's face mask, protective eye wear or face shield need to be used. The operator and assistant should not immediately remove the protective gear as we have seen that aerosol remains suspended in the air even after 3 hours. To further reduce the quantity of aerosol generated high-volume evacuator with a wide bore suction tip should be employed during ultrasonic scaling. The large

bore suction tip with a diameter of 8 mm or more can remove air at the rate of 100 cubic feet per minute, this reduces aerosol and splatter by 93–96% [18]. Disinfecting the oral cavity using mouthwashes could further reduce the bacterial load of the aerosol generated during scaling. In a systematic review, V C Marui observed that pre-procedural rinsing the oral cavity with mouth washes like chlorhexidine, cetylpyridinium chloride or essential oils prior to scaling could result in significantly lower numbers of bacterial CFU's in the dental aerosol [19]. There is also a potential risk for airborne contaminants to enter the ventilation system and spread infection. High efficiency particulate air (HEPA) filters and UV

chambers in the ventilation system can minimize the risk of air contamination [20]. Air disinfection with UV lamp emitting ultra-violet light at 250–265 nm shows bactericidal, fungicidal and viricidal action, the mechanism of action is by the destruction of DNA chains and protein denaturation in the organisms [21].

Limitation of this study was its cross-sectional nature, small sample size and that quantification of individual pathogens was not done. Also, most periodontal pathogens are facultative or obligate anaerobes, hence we cannot directly implicate the periodontal pathogens to cause aerosol-based infections.

5. CONCLUSION

Within the limits of this study, we saw the spreading characteristics of aerosol at different positions in the dental operatory at various time intervals. The patient was in the most contaminated zone followed by the dentist and the assistant. Even after 3 hours after scaling some amount of aerosol remained suspended in the air. The dentist must ensure proper precautionary measures to prevent air-borne nosocomial infections.

ETHICAL APPROVAL

The study protocol was reviewed and approved by the Institutional Ethical Committee and Review Board with an approval number IHEC/SDC/PERIO-1703/21/316.

CONSENT

As per international standard or university standard, patients' written consent has been collected and preserved by the author(s).

ACKNOWLEDGEMENT

The publication was supported by Deanship of scientific research, Prince Sattam bin Abdulaziz University, Al Kharj, Saudi Arabia.

COMPETING INTERESTS

Authors have declared that no competing interests exist.

REFERENCES

1. RE, Miller RL, Mozzarella MA, Ryge G. Studies on dental aerobiology: bacterial

- aerosols generated during dental procedures. *J Dent Res.* 1969;48(1): 49-56.
2. Acharya S, Priya H, Purohit B, Bhatt M. Aerosol contamination in a rural university dental clinic in South India. *Int J Infect Control.* 2010;6:1-7.
3. zymańska J. Dental bioaerosol as an occupational hazard in a dentist's workplace. *Ann Agric Environ Med.* 2007;14(2):203-207.
4. Yamada H, et al. Aerial dispersal of blood-contaminated aerosols during dental procedures. *Quintessence Int.* 2011; 42:399–405.
5. Rautemaa R, Nordberg A, Wuolijoki-Saaristo K, Meurman JH. Bacterial aerosols in dental practice—A potential hospital infection problem? *J Hosp Infect.* 2006;64:76–81.
6. Miller RL. Characteristics of blood-containing aerosols generated by common powered dental instruments. *Am Ind Hyg Assoc J.* 1995;56:670-6.
7. King TB, Muzzin KB, Berry CW, Anders LM. The effectiveness of an aerosol reduction device for ultrasonic scalers. *J Periodontol.* 1997;68:45-9.
8. Legnani P, Checchi L, Pelliccioni GA, DAchille C. Atmospheric contamination during dental procedures. *Quintessence Int.* 1994;25:435-439.
9. Harrel SK, Molinari J. Aerosols and splatter in dentistry; a brief review of the literature and infection control implications. *JADA.* 2004;135(4):429–37.
10. Rosen S, Schmakel D, Schoener M. Incidence of respiratory disease in dental hygienists and dietitians. *Clin Prev Dent.* 1985;7: 24-25.
11. Allsopp J, Basu MK, Browne RM, Burge PS, Matthews JB. Survey of the use of personal protective equipment and prevalence of work related symptoms among dental staff. *Occup Environ Med.* 1997;54:125-134.
12. Veena HR, Mahantesha S, Joseph PA, Patil SR, Patil SH. Dissemination of aerosol and splatter during ultrasonic scaling: a pilot study. *Journal of Infection and Public Health.* 2015;8(3):260.
13. Allison JR, Currie CC, Edwards DC, Bowes C, Coulter J, Pickering K, Kozhevnikova E, Durham J, Nile CJ, Jakubovics N, Rostami N. Evaluating aerosol and splatter following dental procedures: Addressing new challenges

- for oral health care and rehabilitation. *Journal of Oral Rehabilitation*. 2021; 48(1):61-72.
14. Singh A, Manjunath RS, Singla D, Bhattacharya HS, Sarkar A, Chandra N. Aerosol, a health hazard during ultrasonic scaling: A clinico-microbiological study. *Indian Journal of Dental Research*. 2016;1;27(2):160.
 15. Bennett AM, Fulford MR, Walker JT, Bradshaw DJ, Martin MV, Marsh PD. Microbial aerosols in general dental practice. *British Dental Journal*. 2000; 189(12):664-7.
 16. Choi JO, Choi YJ, Nam SH. Study on the prevention of cross-infection by aerosols during scaling. *Biomedical Research*. 2018;29(18):3479-3483.
 17. Zhang R, Li Y, Zhang AL, Wang Y, Molina MJ. Identifying airborne transmission as the dominant route for the spread of COVID-19. *Proceedings of the National Academy of Sciences*. 2020 Jun 11.
 18. Aurangjeb AM, Zaman T, Badruddoza M. Practice of dental surgeons about dental splatter and aerosol. *City Dental College Journal*. 2013;10(2):10-6.
 19. Marui VC, Souto ML, Rovai ES, Romito GA, Chambrone L, Pannuti CM. Efficacy of preprocedural mouthrinses in the reduction of microorganisms in aerosol: A systematic review. *The Journal of the American Dental Association*. 2019;150(12):1015-26.
 20. Micik RE, Miller RL, Mazzarella MA, Ryge G. Studies on dental aerobiology: I. Bacterial aerosols generated during dental procedures. *Journal of Dental Research*. 2007;48(1):49-56.
 21. Szymanska J. Dental bioaerosol as an occupational hazard in a dentist's workplace. *Annals of Agricultural and Environmental Medicine*. 2007;14(2).

© 2021 Inbasekaran et al.; This is an Open Access article distributed under the terms of the Creative Commons Attribution License (<http://creativecommons.org/licenses/by/4.0>); which permits unrestricted use; distribution; and reproduction in any medium; provided the original work is properly cited.

Peer-review history:
The peer review history for this paper can be accessed here:
<https://www.sdiarticle5.com/review-history/82205>